


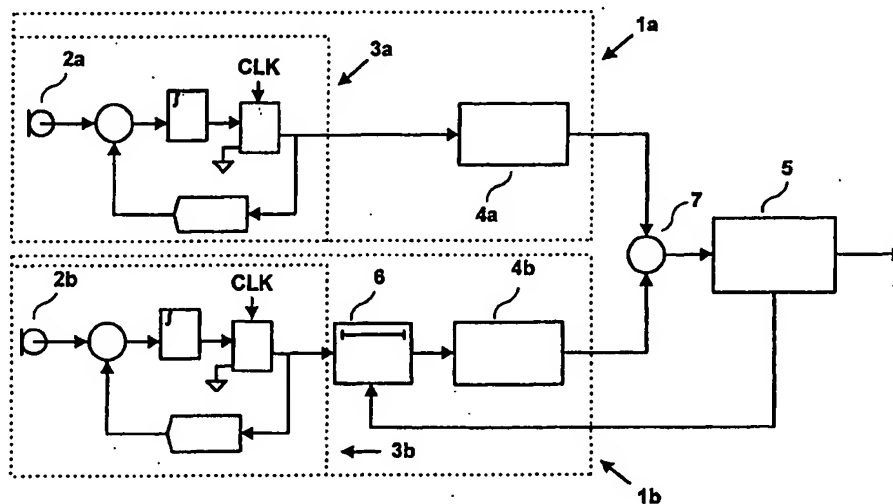

## INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

<b>(51) International Patent Classification <sup>7</sup> :</b>  <b>H04R 25/00</b>	<b>A1</b>	<b>(11) International Publication Number:</b> <b>WO 00/47015</b>  <b>(43) International Publication Date:</b> 10 August 2000 (10.08.00)
<b>(21) International Application Number:</b> PCT/EP99/00767 <b>(22) International Filing Date:</b> 5 February 1999 (05.02.99)  <b>(71) Applicant (for all designated States except US):</b> TØPHOLM & WESTERMANN APS [DK/DK]; Ny Vestergaardsvej 25, DK-3500 Værløse (DK).  <b>(72) Inventors; and</b> <b>(75) Inventors/Applicants (for US only):</b> ANDERSEN, Henning, Hougaard [DK/DK]; Adalsvej 40, DK-2970 Hørsholm (DK). LUDVIGSEN, Carl [DK/DK]; Borghaven 19, DK-2500 Valby (DK).  <b>(74) Agent:</b> BÖHMER, Hans, Erich; Keplerstrasse 23, D-71134 Aildlingen (DE).		<b>(81) Designated States:</b> AU, CA, JP, US, European patent (AT, BE, CH, CY, DE, DK, ES, FI, FR, GB, GR, IE, IT, LU, MC, NL, PT, SE).  <b>Published</b> <i>With international search report.</i>

**(54) Title:** HEARING AID WITH BEAM FORMING PROPERTIES**(57) Abstract**

The invention relates to a hearing aid with beam forming properties, having at least two microphone channels (1a, 1b) for at least two microphones (2a, 2b), said microphone channels comprising each an analog to digital converter (3a, 3b) and having at least one programmable or program controlled signal processor (5), as well as a digital to analog converter, and at least one receiver and a battery for power supply. The invention particularly comprises in each microphone channel (1a, 1b) a sigma-delta-type analog to digital converter (3a, 3b) including a digital low pass filter and a decimator (4) for converting a 1 Bit Stream of a high clock frequency into a digital word sequence of a lower clock frequency. At least one of said at least two microphone channels contains a controllable delay device (6) connected to the input side of the respective digital low pass filter and decimator (4) of said channel, said delay device (6) being controllable by said at least one signal processor (5). Preferably the delay device (6) is integrated into said sigma-delta-ADC (3).

**FOR THE PURPOSES OF INFORMATION ONLY**

Codes used to identify States party to the PCT on the front pages of pamphlets publishing international applications under the PCT.

AL	Albania	ES	Spain	LS	Lesotho	SI	Slovenia
AM	Armenia	FI	Finland	LT	Lithuania	SK	Slovakia
AT	Austria	FR	France	LU	Luxembourg	SN	Senegal
AU	Australia	GA	Gabon	LV	Latvia	SZ	Swaziland
AZ	Azerbaijan	GB	United Kingdom	MC	Monaco	TD	Chad
BA	Bosnia and Herzegovina	GE	Georgia	MD	Republic of Moldova	TG	Togo
BB	Barbados	GH	Ghana	MG	Madagascar	TJ	Tajikistan
BE	Belgium	GN	Guinea	MK	The former Yugoslav Republic of Macedonia	TM	Turkmenistan
BF	Burkina Faso	GR	Greece			TR	Turkey
BG	Bulgaria	HU	Hungary	ML	Mali	TT	Trinidad and Tobago
BJ	Benin	IE	Ireland	MN	Mongolia	UA	Ukraine
BR	Brazil	IL	Israel	MR	Mauritania	UG	Uganda
BY	Belarus	IS	Iceland	MW	Malawi	US	United States of America
CA	Canada	IT	Italy	MX	Mexico	UZ	Uzbekistan
CF	Central African Republic	JP	Japan	NE	Niger	VN	Viet Nam
CG	Congo	KE	Kenya	NL	Netherlands	YU	Yugoslavia
CH	Switzerland	KG	Kyrgyzstan	NO	Norway	ZW	Zimbabwe
CI	Côte d'Ivoire	KP	Democratic People's Republic of Korea	NZ	New Zealand		
CM	Cameroon			PL	Poland		
CN	China	KR	Republic of Korea	PT	Portugal		
CU	Cuba	KZ	Kazakstan	RO	Romania		
CZ	Czech Republic	LC	Saint Lucia	RU	Russian Federation		
DE	Germany	LI	Liechtenstein	SD	Sudan		
DK	Denmark	LK	Sri Lanka	SE	Sweden		
EE	Estonia	LR	Liberia	SG	Singapore		

## Hearing aid with beam forming properties

The invention relates to a hearing aid with beam forming properties in accordance with the preamble of claim 1.

Beam forming using at least two or more spaced apart microphones has been known for many years.

### Background of the invention

In the EP 0820210 A2 a method and apparatus for beam forming of the microphone characteristic has been disclosed, by which a pre-determined characteristic of amplification in dependency of the direction from which acoustical signals are received at two spaced apart microphones is formed in that repetitively a mutual delay signal is determined from the output signals of the microphones and according to the reception delay of the microphones, one of the output signals is filtered, thereby the filtering transfer characteristic is controlled in dependency of the mutual delay signal. The output signal of the filtering is exploited as electrical reception signal.

Thus, in principle the time delay or phase lag between the two output signals of the two microphones is used for a beam forming operation.

In a digital hearing aid the single samples are taken with a time difference equally divided by the sampling frequency, f.i. normally  $32 \mu$  sec. The desired delay between two or more microphone signals are typically less than  $32 \mu$  sec, e.g.  $15 \mu$  sec. A way to obtain a delay which is less than one sample is to have the DSP interpolate signal values between two samples with a certain delay and use those delayed sample values in the further processing. But this requires many calculations and takes up valuable space and power in the DSP.

Also, the signal will be somewhat distorted as the delayed samples are not "true" samples.

However, for an active control of beam forming properties in a directional hearing aid, the delays that could be realized, based on the sample frequency and conventional shift register technology would be much too long to be useful.

in order to realize sample delays as low as 1  $\mu$  sec the conventional technology can not be used.

Thus, it is an object of the present invention to create a novel hearing aid with beam forming properties in which an active control of the delay of at least one of the incoming signals of a hearing aid having at least two microphones can be used for active beam forming. With such a hearing aid a great number of various directional orientations of hearing aids could actively and controllably be realized.

Particularly, by using faster sampling rates, the samples because of their shorter time intervals could be used directly, so that desirable short delays could be realized.

By using a sigma-delta converter with a sampling rate or clock frequency of f.i. 1 MHz and by inserting a 1 bit adjustable and controllable digital delay line in the bit stream from one of the sigma-delta converters to the corresponding decimator filter of the converter one could obtain delayed difference steps of multiples of 1  $\mu$  sec, which could not be achieved with conventional hearing aid technology.

#### Summary of the invention

For this purpose a new hearing aid with beam forming properties has been developed, which has at least two microphone channels for at least two microphones, said microphone channels containing each an

analog to digital converter, and having at least one programmable or programmed digital signal processor, as well as a digital to analog converter, at least one receiver and a battery for power supply.

This new hearing aid, in accordance with the present invention, contains in each of said microphone channels a sigma-delta-type analog to digital converter including a digital low pass filter and decimator filter for converting a 1 bit stream of a high clock frequency into a digital word sequence of a lower clock frequency, whereby at least one of said at least two microphone channels contains a controllable delay device connected to the input side of the respective digital low pass filter and decimator filter of said channel, said delay device being controllable by said at least one digital signal processor.

It is advantageous to have said delay device integrated into the sigma-delta ADC.

It is of particular importance to use, as a delay device, a programmable or program controlled tapped shift register for realizing various different delays of the bit stream signals before their entering the respective digital low pass filter and decimator. In order to realize controllable delays as short as 1  $\mu$  sec it is of advantage to use a clock frequency for the sigma delta ADC in the range of 1 MHz or even higher and a clock frequency in the area of 10 to 50 kHz for the digital low pass filter and decimator filter.

It is now obvious that with such a configuration of the input side of a beam forming hearing aid with active beam control various additional possibilities exist which are subject of the remaining claims. Particularly, by this new hearing aid a very high resolution delay may be achieved.

### Brief description of the drawings

The invention will now be described in more detail in conjunction with several embodiments and the accompanying drawings:

In the drawings

Fig. 1 shows schematically a number of polar diagrams of variations of beam directions which could be realized by the present invention;

Fig. 2 shows schematically the general structure of a sigma-delta analog to digital converter (ADC);

Fig. 3 shows schematically a first embodiment of the invention;

Figs. 4, 5, 6 and 7 show schematically further embodiments of the invention.

Fig. 1 illustrates four different directional patterns in polar diagrams.

Fig. 1a represents the hypercardioid system which has a very desirable directional effect. 1b is the bidirectional system which has no delay for any of the two microphones and therefore attenuates all sounds coming directly from the sides (90 degrees and 270 degrees) as the two microphones level out each other. 1c is the cardioid which must have a delay in the front microphone equal to the longitudinal delay between the inlet ports of the two microphones. Finally, 1d is the omnidirectional or spherical system, which is simply a single microphone (the other microphone is switched off), or the two microphone signals are added and not subtracted from each other.

However, by controlling the various delay devices, other directional patterns could be realized. This will be more evident from the following description of the Figs. 2 to 7.

Detailed description of preferred embodiments of the invention

As has been explained above, for realizing hearing aids in accordance with the present invention, normal analog to digital converters operating with clock frequencies of 16 or 32 kHz could not be used for realizing delays in the range of 1  $\mu$ sec or multiples thereof.

Fig. 2 shows a well known type of a first order sigma-delta digital to analog converter comprising basically a summing circuit, an integrator, a comparator stage (1 bit ADC) and a digital low pass filter and a decimator filter. The comparator stage is controlled by a high frequency clock generator supplying clock pulses in the area of 1MHz or higher. The output of the integrator is connected also to a 1 bit DAC, the output of which is connected to a second input of the summing circuit. The digital low pass filter and decimator filter operates at a clock frequency of f.i. 32 kHz and converts the 1 bit stream of a clock frequency of about 1 MHz into a sequence of data words at the lower frequency, f.i. 16 or 32 kHz. These data words could e.g. be 20 bit wide. These data words are then, normally, applied to a programmable or program controlled digital signal processor.

It is to be understood that all embodiments of the invention will make use of such sigma-delta-type ADC's, provided a high clock frequency in the area of 1 MHz or higher is used for controlling the comparator.

Fig. 3 shows, schematically, a first example of the inventive conceptual design.

Two microphone channels 1a and 1b comprise microphones 2a and 2b

and sigma-delta analog to digital converters 3a, 3b including digital low pass filters and decimator filters 4a and 4b for supplying data words to a programmable or program controlled digital signal processor 5.

In one of the microphone channels a controllable delay device 6 is included. This delay device is typically a multiple tap shift register and the control signal coming from the DSP 5 will decide how many 1 bit stages each sample of the bit stream will go through (and thus be delayed by) before they are tapped and sent further on in the system, in this case to the digital low pass filter and decimator 4. The resulting delay is equal to the number of stages times the inverse sampling rate, f.i. 1 MHz.

With this high resolution of the sigma-delta ADC the time resolution can be 30 - 40 times higher than would be possible inside the DSP using its clock as a basis for delays. Normally, this setup can only handle beam forming from the front or from the back but not both. The controllable delay would be controlled by the DSP so that the DSP direct the beam in the desired directions.

Fig. 4 shows a further embodiment of the invention. All parts and components which are the same as in Fig. 3 are designated with the same reference numerals and need not to be described again. This holds true for all other Figs. as well so that only the differences will be explained in detail.

In Fig. 4 both microphone channels 1a and 1b contain each a controllable delay device 6a, 6b. They can, of course, be controlled independently and separately. Although two delay devices are included, only one of the two may be controlled whereas the other is switched off.

The output signals of the digital low pass filter and decimator filters 4a and 4b are combined in a summing circuit 7 and passed on to the DSP. Thus, by having controllable delays in both sigma-delta converters



it will be possible to reverse the beam forming operation and use it both at front and back.

In Fig. 5, which in almost all respects is similar to Fig. 4, the output signal of the lower one of the two microphone channels 1b is now connected to a first input of a multiplier stage 8, the second input of which receives a controlling input from the DSP.

The output of the multiplier stage 8 is applied to the second input of the summing circuit 7, which feeds into the DSP.

It may be desirable to make a shift from e.g. the hypercardioid to the omnidirectional characteristic. For this purpose the multiplier 8 is added after the digital low pass filter and decimator filter for one microphone or for both. The DSP then can multiply the samples with factors between -1 and +1.

Fig. 6 shows the extension from two microphone channels to multiple microphone channels. Again, controllable delay devices may be arranged in one channel, in two channels or in all channels. The output signals of all channels are combined in a combination circuit 9, the output signals of which are applied to the DSP. This combination could be effected with different factors between -1 to +1, if convenient.

Fig. 7 finally, shows another variation of the inventive circuit in which at least one of the microphone channels has not only one delay device and one digital low pass filter and decimator filter but two of those in parallel. It is also conceivable to have these parallel arrangements in one or more channels, even in all of them.

It is also possible to use more than two delay devices in parallel in at least one of said microphone channels, all connected to their respective digital low pass filter and decimator filter of said at least one of said channels.

## P A T E N T C L A I M S

1. Hearing aid with beam forming properties, having at least two microphone channels (1a, 1b) for at least two microphones (2a, 2b), said microphone channels comprising each an analog to digital converter (3a, 3b) and having at least one programmable or program controlled signal processor (6), as well as a digital to analog converter, and at least one receiver and a battery for power supply, characterized in that each microphone channel (1a, 1b) contains a sigma-delta-type analog to digital converter (3a, 3b) including a digital low pass filter and decimator (4) for converting a 1 Bit stream of a high clock frequency into a digital word sequence of a lower clock frequency, and that at least one of said at least two microphone channels contains a controllable delay device (6) connected to the input side of the respective digital low pass filter and decimator (4) of said channel, said delay device (6) being controllable by said at least one signal processor (5).
2. Hearing aid in accordance with claim 1, characterized in that the delay device (6) is integrated into said sigma-delta-ADC (3).
3. Hearing aid in accordance with claim 1 or 2, characterized in that a first order sigma-delta converter is used in said at least two microphone channels.
4. Hearing aid in accordance with claims 1 or 2, characterized in that a second order or even higher order sigma-delta-converter is used in said at least two microphone channels.
5. Hearing aid in accordance with claims 1 to 3, characterized in that the clock frequency for the sigma-delta-ADC (3)

is in the range of 1 MHz or higher and that said lower frequency for the digital word sequence is in the range of 10 to 50 kHz.

6. Hearing aid in accordance with claim 1 characterized in that said at least one delay device comprises a programmable or program controlled tapped shift register for realizing various different delays of said bit stream signals before their entering said digital low pass filter and decimator.
7. Hearing aid in accordance with claims 1 to 6, characterized in that the output signals of said at least two microphone channels may be combined directly in the DSP including further processing or filtering of said output signals.
8. Hearing aid in accordance with claims 1 to 6, characterized in that the output signals of said at least two microphone channels are combined in a summing circuit (7) for controlling said digital signal processor.
9. Hearing aid in accordance with claim 1, characterized in that in each sigma-delta converter (3a, 3b) of said at least two microphone channels (1a, 1b) a controllable delay device (6a, 6b) is included.
10. Hearing aid in accordance with claims 1 to 9, characterized in that one of said at least two microphone channels is directly connected to the summing circuit (7), whereas the other of said two microphone channels is connected to a first input of a multiplier stage (8), the output of which is coupled to said summing circuit (7), whereas a second input of said multiplier stage (8) is controlled by the digital signal processor (5).
11. Hearing aid in accordance with claim 1, characterized by multiple microphone channels, most of them or all of them being equipped

with sigma-delta analog to digital converters (3) including at least in some of them said controllable delay devices, the outputs of which are combined in a combination circuit, such as an integrator circuit or combination circuit (9) connected to the input side of said at least one digital signal processor (5).

12. Hearing aid in accordance with claim 1, characterized in that at least one of the said at least two microphone channels is equipped with a sigma-delta analog to digital converter including at least two delay devices in parallel operating on two digital low pass filters and decimators, the output signals of all said digital low pass filters and decimators are being combined in an combination circuit connected to the input side of said at least one digital signal processor, or are directly connected to the said signal processor as individual or separate signals.
13. Hearing aid in accordance with claim 1, characterized by a remote control unit for controlling the said digital signal processor for effecting various beam forming directional orientations of said at least two microphones by influencing one or more of said delay devices for introducing various different delays.

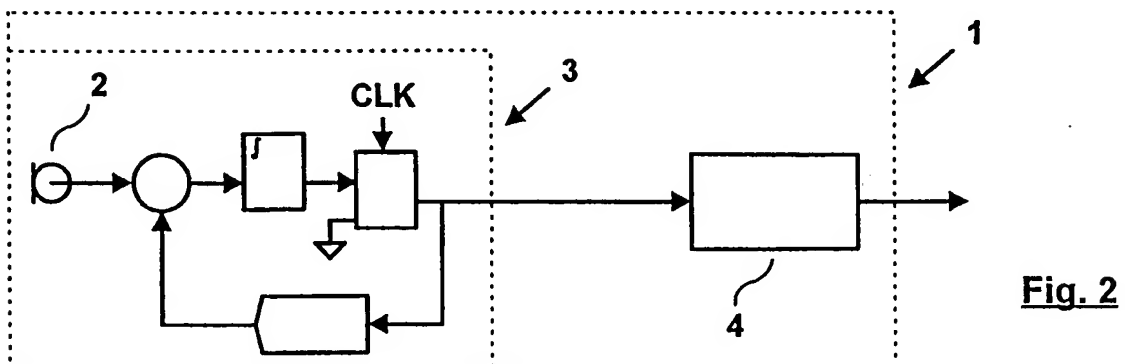
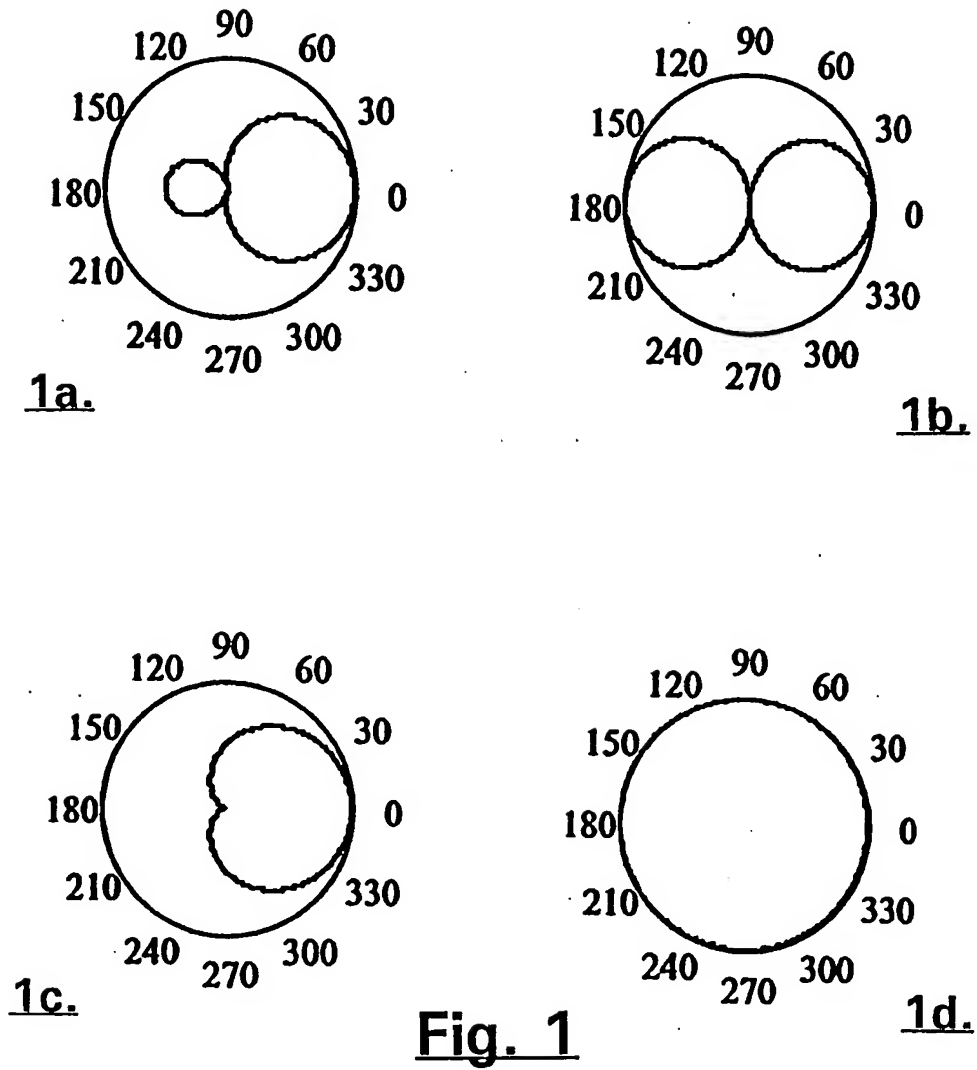


Fig. 3




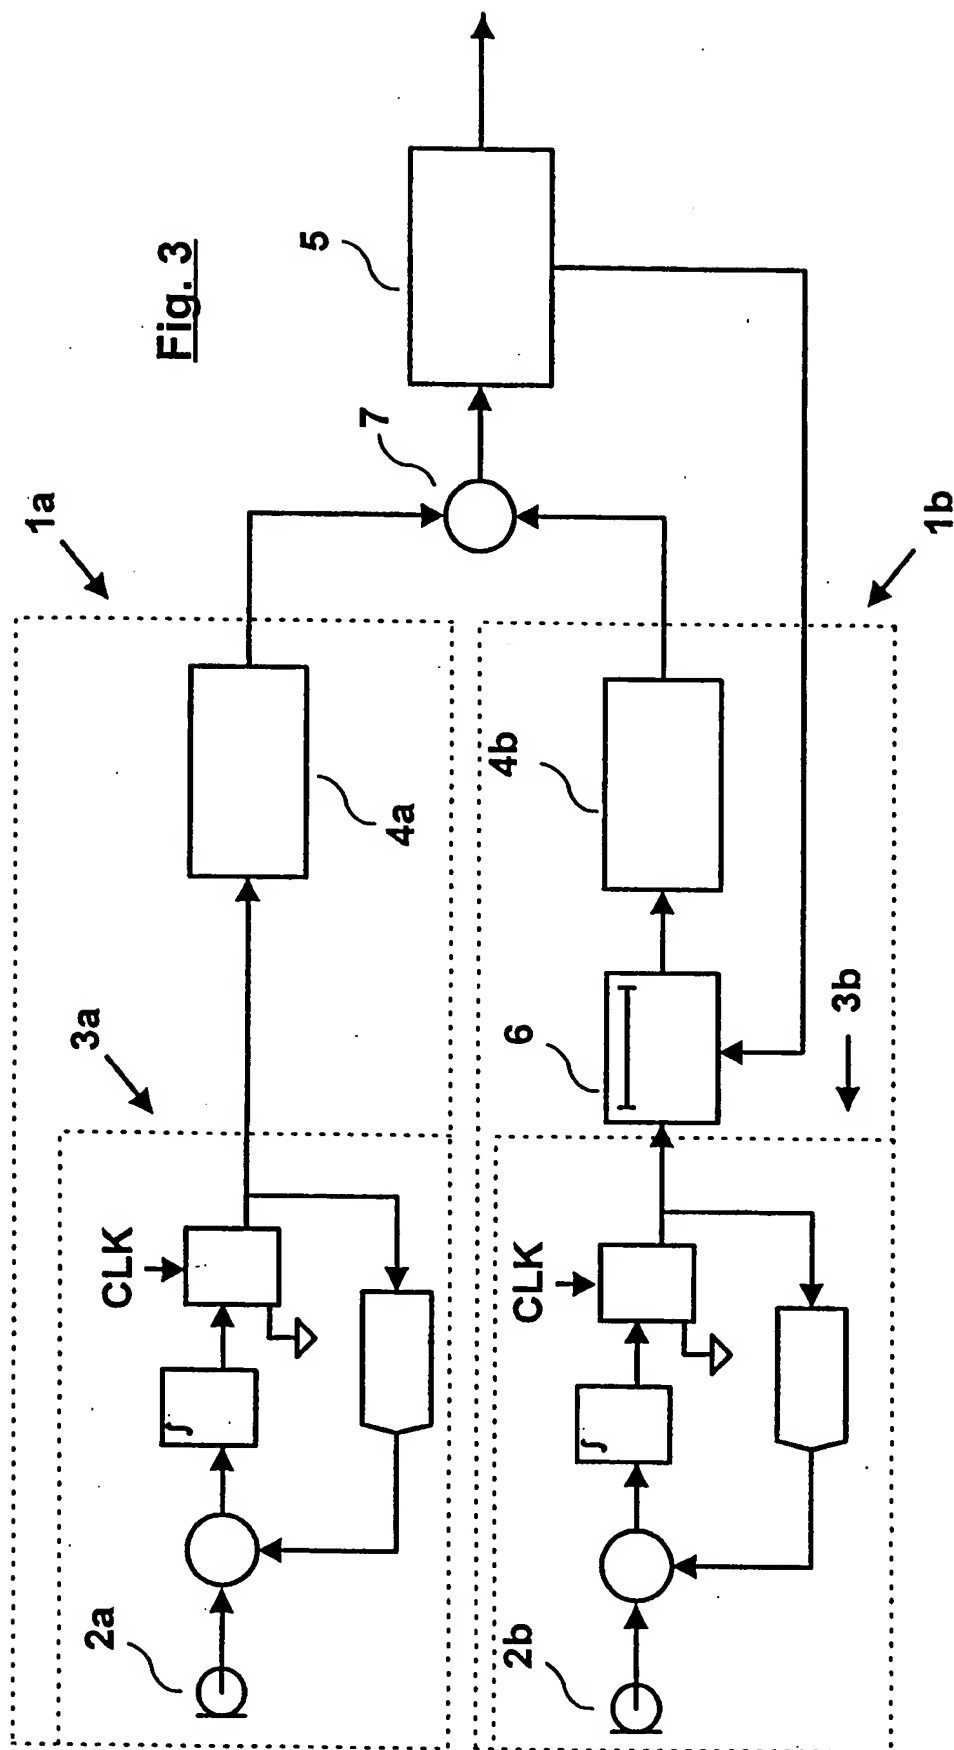



Fig. 4



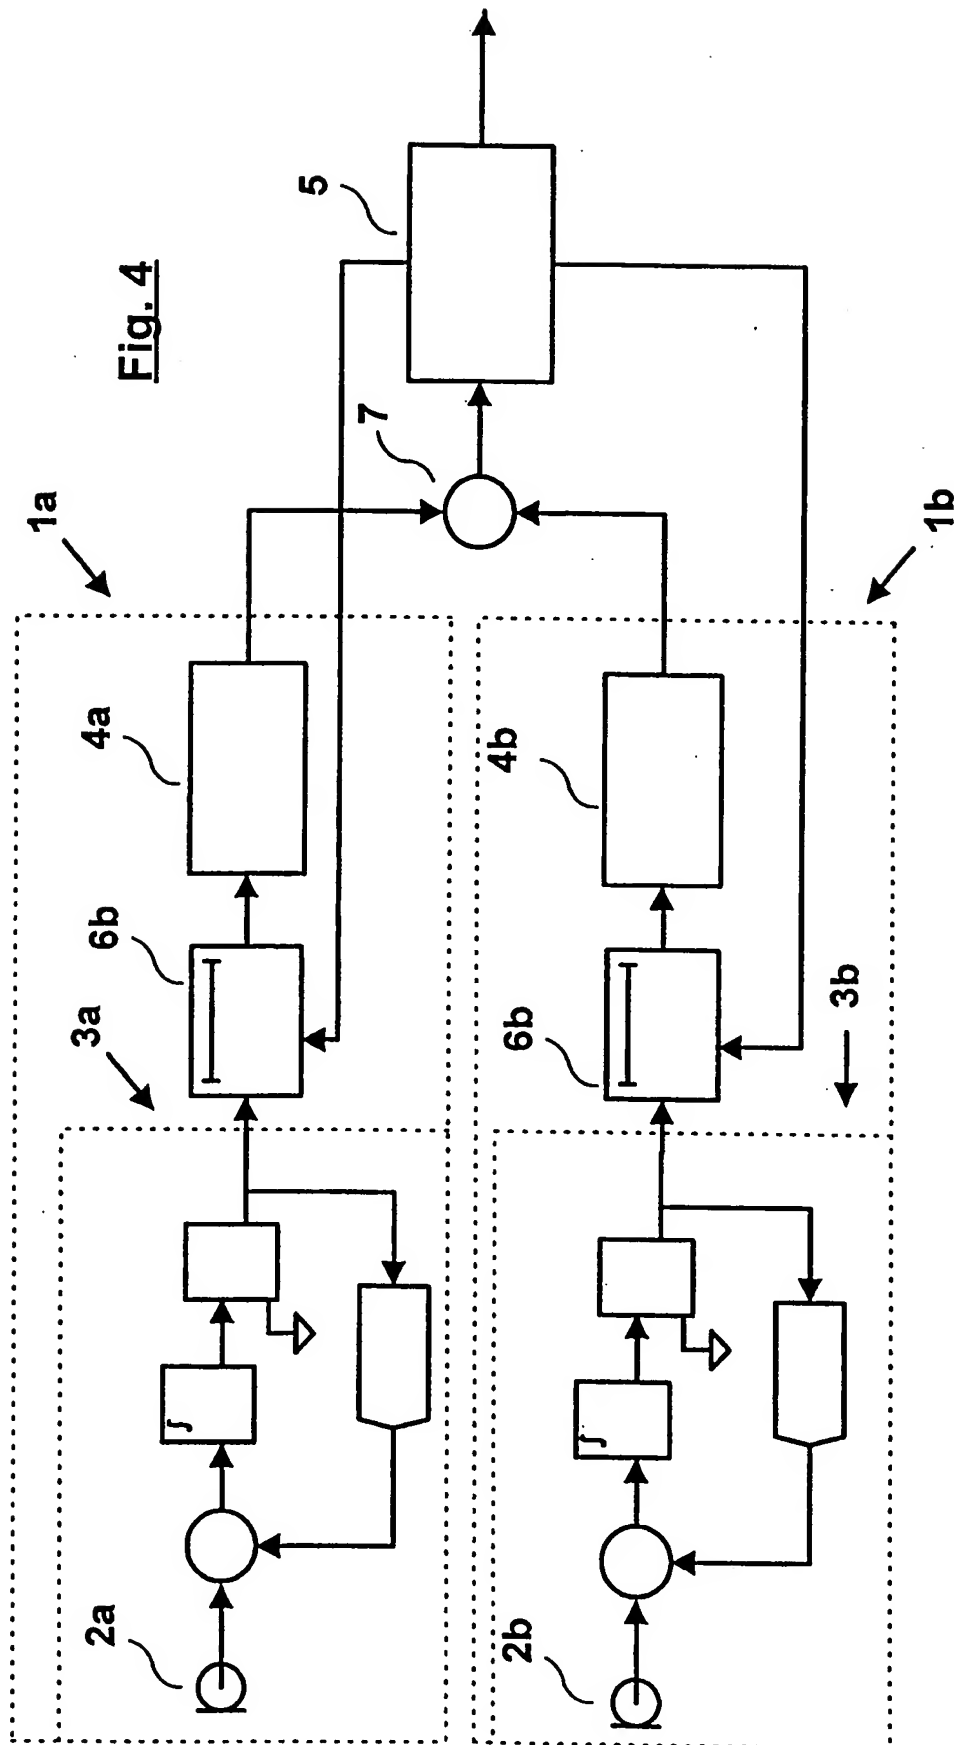

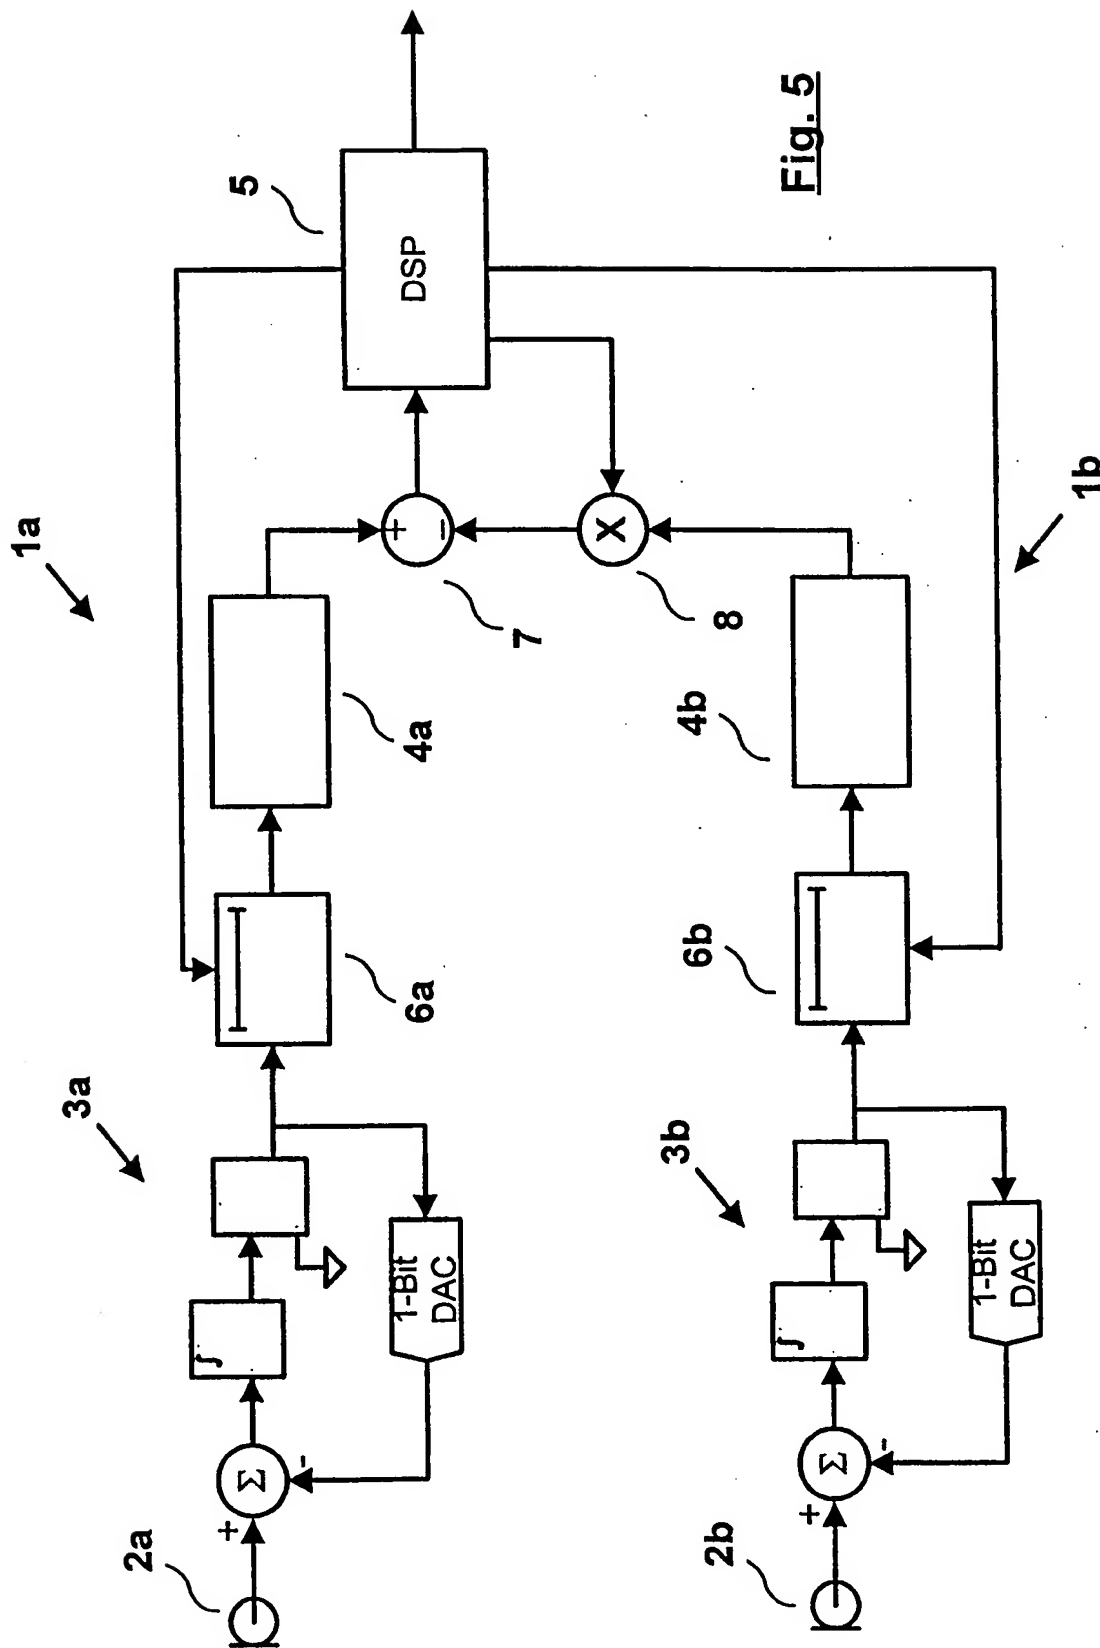

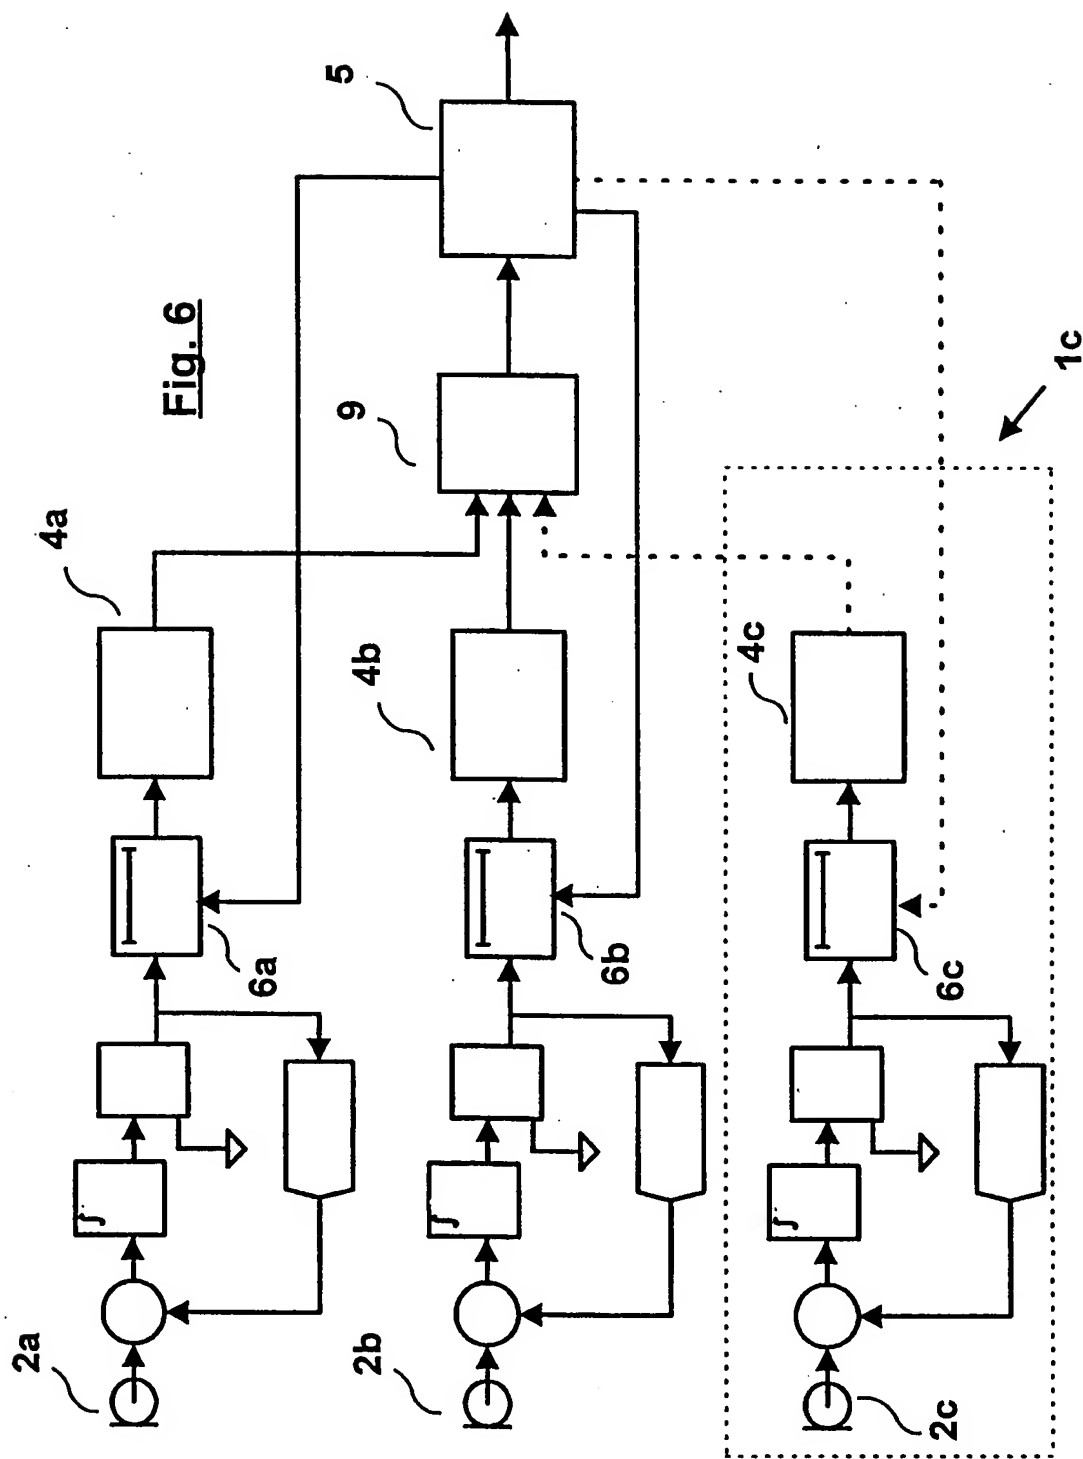

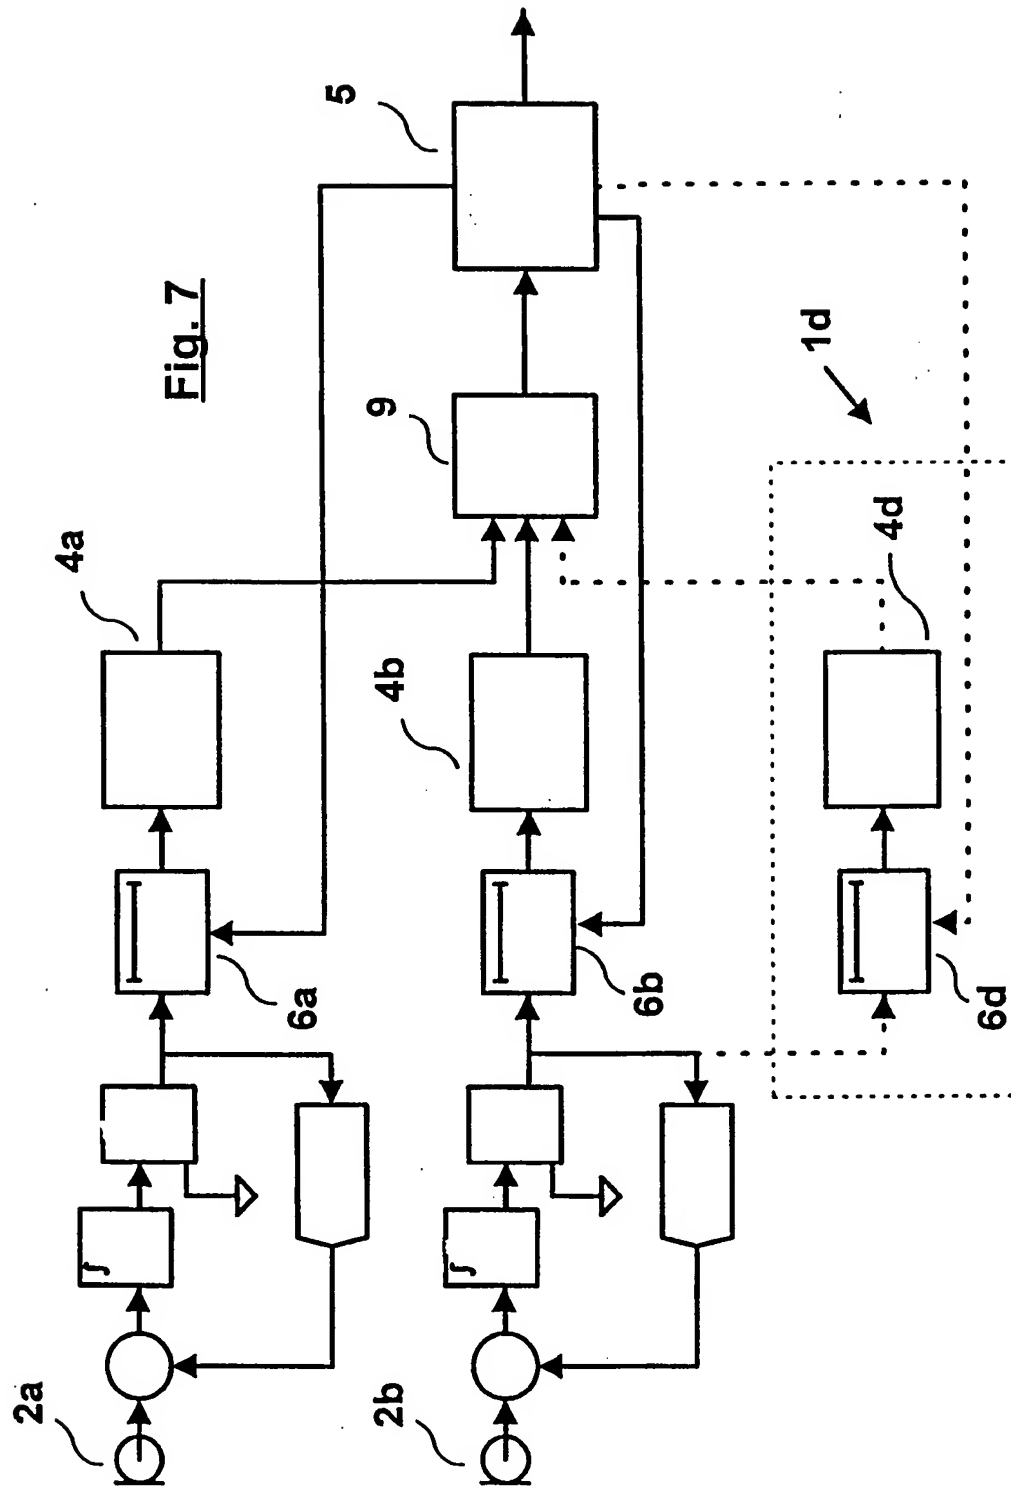

## INTERNATIONAL SEARCH REPORT

International Application No

PCT/EP 99/00767

## A. CLASSIFICATION OF SUBJECT MATTER

IPC 7 H04R25/00

According to International Patent Classification (IPC) or to both national classification and IPC

## B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)

IPC 7 H04R H03M H03H

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Electronic data base consulted during the international search (name of data base and, where practical, search terms used)

## C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category *	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
Y A	WO 98 47227 A (LAMAR SIGNAL PROCESSING) 22 October 1998 (1998-10-22) page 1, line 10-21 page 2, line 6-14 page 7, line 34 -page 13, line 9 ---	1,3,5-8, 11,12 2,9,10
Y A	DE 44 41 996 A (TOEPHOLM & WESTERMANN) 30 May 1996 (1996-05-30) column 2, line 29 -column 4, line 44 ---	1,3,5-8, 11,12 2,9
A	WO 96 16482 A (ANALOG DEVICES) 30 May 1996 (1996-05-30) page 1, line 14-25 page 2, line 26-33 page 3, line 6 -page 4, line 8 page 4, line 25 -page 8, line 2 ---	1-3,5, 11,12
	--- -/--	

☒ Further documents are listed in the continuation of box C.☒ Patent family members are listed in annex.

## \* Special categories of cited documents:

"A" document defining the general state of the art which is not considered to be of particular relevance

"E" earlier document but published on or after the international filing date

"L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)

"O" document referring to an oral disclosure, use, exhibition or other means

"P" document published prior to the international filing date but later than the priority date claimed

"T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention

"X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone

"Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art.

"&amp;" document member of the same patent family

Date of the actual completion of the international search

1 October 1999

Date of mailing of the international search report

12/10/1999

Name and mailing address of the ISA

European Patent Office, P.B. 5818 Patentlaan 2  
NL - 2280 HV Rijswijk  
Tel. (+31-70) 340-2040, Tx. 31 651 epo nl,  
Fax: (+31-70) 340-3016

Authorized officer

Zanti, P

## INTERNATIONAL SEARCH REPORT

International Application No

PCT/EP 99/00767

## C.(Continuation) DOCUMENTS CONSIDERED TO BE RELEVANT

Category *	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
A	US 5 305 004 A (FATTARUSO) 19 April 1994 (1994-04-19) abstract figure 1 -----	1,4
A	DE 36 42 828 A (TOEPHOLM & WESTERMANN) 13 August 1987 (1987-08-13) figure 1 column 3, line 52-68 column 6, line 42 -column 7, line 3 -----	1,13

# INTERNATIONAL SEARCH REPORT

Information on patent family members

International Application No

PC1/EP 99/00767

Patent document cited in search report	Publication date	Patent family member(s)	Publication date
WO 9847227 A	22-10-1998	AU 6933098 A	11-11-1998
DE 4441996 A	30-05-1996	AT 166199 T	15-05-1998
		AU 691001 B	07-05-1998
		AU 2671495 A	19-06-1996
		CA 2204757 A	06-06-1996
		DE 59502189 D	18-06-1998
		WO 9617493 A	06-06-1996
		EP 0793897 A	10-09-1997
		JP 10504155 T	14-04-1998
		US 5878146 A	02-03-1999
WO 9616482 A	30-05-1996	US 5619202 A	08-04-1997
		DE 69510083 D	08-07-1999
		EP 0793876 A	10-09-1997
		US 5625358 A	29-04-1997
		US 5625359 A	29-04-1997
		US 5528240 A	18-06-1996
		US 5574454 A	12-11-1996
		US 5552785 A	03-09-1996
US 5305004 A	19-04-1994	JP 6244734 A	02-09-1994
DE 3642828 A	13-08-1987	CH 672215 A	31-10-1989
		DK 41087 A	04-08-1987
		IT 1202432 B	09-02-1989
		JP 1914001 C	23-03-1995
		JP 6040680 B	25-05-1994
		JP 62248400 A	29-10-1987
		US 4947432 A	07-08-1990